



# Corrigendum: Voice Pathology Detection Using Modulation Spectrum-Optimized Metrics

## OPEN ACCESS

Laureano Moro-Velázquez\*, Jorge Andrés Gómez-García and Juan Ignacio Godino-Llorente

### Edited and Reviewed by:

Adam P. Vogel,  
University of Melbourne, Australia

### \*Correspondence:

Laureano Moro-Velázquez  
laureano.moro@upm.es

Received: 21 July 2016

Accepted: 02 August 2016

Published: 24 August 2016

### Citation:

Moro-Velázquez L, Gómez-García JA and Godino-Llorente JI (2016) Corrigendum: Voice Pathology Detection Using Modulation Spectrum-Optimized Metrics. *Front. Bioeng. Biotechnol.* 4:67. doi: 10.3389/fbioe.2016.00067

Center for Biomedical Technology, Universidad Politécnica de Madrid, Madrid, Spain

**Keywords:** modulation spectrum, speech, dysphonia, cross-validation, EER


## A corrigendum on

### Voice Pathology Detection Using Modulation Spectrum-Optimized Metrics

by Moro-Velázquez, L., Gómez-García, J. A., and Godino-Llorente, J. I. (2016). *Front. Bioeng. Biotechnol.* 4:1. doi:10.3389/fbioe.2016.00001

### Reason for Corrigendum:

There is a mistake in the values of the  $x$  axis of **Figure 5** as published. The correct version of **Figure 5** appears below. The article says that all tests have been performed in the range 20–200 ms but in **Figure 5**,  $x$  axis only includes the range 20–120 ms. The new figure includes the appropriate axis values. The authors apologize for the mistake. This error does not change the scientific conclusions of the article in any way.

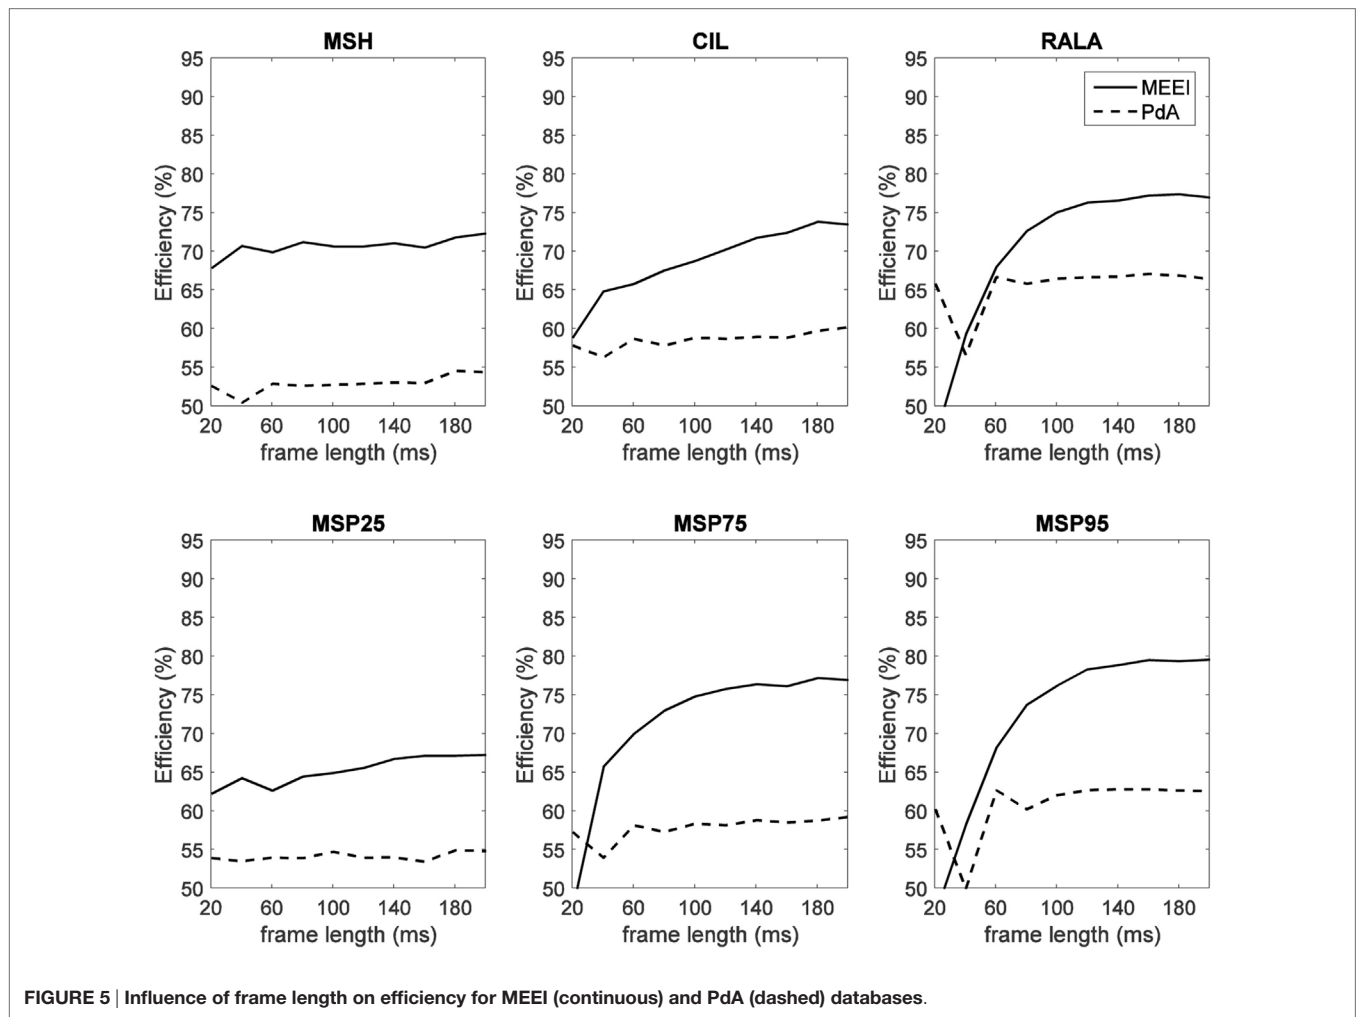

**Conflict of Interest Statement:** The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

Copyright © 2016 Moro-Velázquez, Gómez-García and Godino-Llorente. This is an open-access article distributed under the terms of the Creative Commons

Attribution License (CC BY). The use, distribution or reproduction in other forums is permitted, provided the original author(s) or licensor are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms.